

Accessories, disposables and software options

ulrich medical® contrast media injectors for MRI and CT



The simple
ordering overview

Ulrich
medical

Contents

| | | | Page |
|---|--|--|------|
|  | MaxTM 3 ulricheasyINJECT | MRI contrast media injector | 4 |
|  | MaxTM 2M ulricheasyINJECT | MRI contrast media injector | 7 |
|  | ulrichINJECT <i>CT motionTM</i> | CT contrast media injector | 10 |
|  | XD 200x injectors missouri TM mississippi TM ohio M TM ohio <i>tandem</i> TM tennessee TM | CT and MRI contrast media injectors | 13 |
| | | Overview of product numbers, accessories, disposables and soft- ware options | 17 |



MRI contrast media injector

Accessories

Product number

Convenience package

consisting of waste bin, tray and media rod

XD 10500



Drip cup

Packaging unit (PU) 5 items

XD 10740



Adapter ring for small bottles

PU 100 items

For contrast media bottles with bottle neck diameter of 21 mm for adapting to an Easy-Click-Cassette holder | contrast media spike

XD 10741



Pair of holding arms

SP002808-ET



Bottle holder multiuse

SP001612-ET



Power cable extension

5.0 m

XD 2068-00 IEC

Power supply cable

- Power supply cable CEE 7 Europe 2.0 m XD 2068-01
- Power supply cable BS1363 GB 2.0 m XD 2068-02
- Power supply cable GB2099 CN 2.0 m XD 2068-03
- Power supply cable NBR14136 BR 2.5 m XD 2068-04
- Power supply cable SANS164 RSA 1.5 m XD 2068-05
- Power supply cable NEMA5-15 US 3.0 m XD 2068-06
- Power supply cable SEV Type 12 CH 2.5 m XD 2068-07
- Power supply cable CEI 23-50 ITA 1.5 m XD 2068-08
- Power supply cable AS3112 AUS 2.0 m XD 2068-09

MRI contrast media injector

MaxTM 3
ulricheasyINJECT

Disposables

Product number

Easy-Click-Cassette Max. 3TM

24 h, PU 40 items


- With holder s for contrast media bottles with a bottle neck diameter of 21 mm XD 10710
- With holder l for contrast media bottles with a bottle neck diameter of 33 mm XD 10711



Easy-Click-Cassette Max. 3TM – flex

24 h, PU 40 items

- Spike for CT (CM/NaCl), MRI (NaCl), PU 30 items XD 10704
- Spike for MRI (CM) – holder l XD 10705
With holder l for contrast media bottles with a bottle neck diameter of 33 mm, PU 30 items
- Spike for MRI (CM) – holder s XD 10706
With holder s for contrast media bottles with a bottle neck diameter of 21 mm, PU 30 items



Patient tubing

PU 100 items

- 250 cm XD 10701
- 320 cm XD 10702



Patient tubing system

XD 10707

For the use of pre-filled contrast media syringes

PU 50 items

Consisting of

- Patient tubing connector (XD 10703)
- Patient tubing 320 cm (XD 2045)





MRI contrast media injector

Software options Product number

| Software options | Product number | |
|--------------------------------|----------------|--|
| Max 3™ software package | XD 10600 | Consisting of CM-Select, Same patient and Vein-check |
| Same patient | XD 10630 | Multiple examinations on a patient without changing patient tubing |
| CM-Select | XD 10640 | <ul style="list-style-type: none"> Careful selection of a second contrast medium (two different contrast media are available simultaneously) Possibility to change the type of contrast medium on the media slots by means of NaCl rinsing (no need to change the Easy-Click-Cassette)** |
| Vein-check | XD 10650 | Checking the correct position of the cannula in the patient |

** see instructions for use Max 3™

MRI contrast media injector

MaxTM 2M
ulricheasyINJECT

Accessories

Product number

Convenience package

Consisting of waste bin, tray and media rod

XD 10500



Drip cup

PU 5 items

XD 10740



Adapter ring for small bottles

PU 100 items

For contrast media bottles with bottle neck diameter of 21 mm for adapting to an Easy-Click-Cassette holder | contrast media spike

XD 10741



Pair of holding arms

SP002808-ET



Bottle holder multiuse

SP001612-ET



Power cable extension

5.0 m

XD 2068-00 IEC

Power supply cable

- Power supply cable CEE 7 Europe 2.0 m XD 2068-01
- Power supply cable BS1363 GB 2.0 m XD 2068-02
- Power supply cable GB2099 CN 2.0 m XD 2068-03
- Power supply cable NBR14136 BR 2.5 m XD 2068-04
- Power supply cable SANS164 RSA 1.5 m XD 2068-05
- Power supply cable NEMA5-15 US 3.0 m XD 2068-06
- Power supply cable SEV Type 12 CH 2.5 m XD 2068-07
- Power supply cable CEI 23-50 ITA 1.5 m XD 2068-08
- Power supply cable AS3112 AUS 2.0 m XD 2068-09





MRI contrast media injector

Disposables

Product number

Easy-Click-Cassette Max. 2MTM

24 h, PU 40 items


- With holder s for contrast media bottles with a bottle neck diameter of 21 mm XD 10712
- With holder l for contrast media bottles with a bottle neck diameter of 33 mm XD 10713



Easy-Click-Cassette Max. 2MTM – flex

24 h, PU 40 items

- Spike for CT (CM/NaCl), MRI (NaCl), PU 30 items XD 10704
- Spike for MRI (CM) – holder l XD 10705
- With holder l for contrast media bottles with a bottle neck diameter of 33 mm, PU 30 items
- Spike for MRI (CM) – holder s XD 10706
- With holder s for contrast media bottles with a bottle neck diameter of 21 mm, PU 30 items



Patient tubing

PU 100 items

- 250 cm XD 10701
- 320 cm XD 10702



Patient tubing system

XD 10707

For the use of pre-filled contrast media syringes

PU 50 items

Consisting of

- Patient tubing connector (XD 10703)
- Patient tubing 320 cm (XD 2045)



MRI contrast media injector

MaxTM 2M
ulricheasyINJECT

| Software options | Product number | |
|------------------|----------------|--|
|------------------|----------------|--|

| | | |
|---|----------|---|
| Max 2MTM software package | XD 10610 | Consisting of Same patient and Vein-check |
|---|----------|---|

| | | |
|---------------------|----------|--|
| Same patient | XD 10630 | Multiple examinations on a patient without changing patient tubing |
|---------------------|----------|--|

| | | |
|-------------------|----------|---|
| Vein-check | XD 10650 | Checking the correct position of the cannula in the patient |
|-------------------|----------|---|



ulrichINJECT CT motion™

CT contrast media injector



Accessories

Product number

Waste bin

XD 8018



Drip cup
PU 5 items

XD 10740



NaCl rod

XD 8163



Tray

XD 8021



Tube insertion device

XD 8090



Protective cap for particle filter holder

XD 8118



Bottle holder

SP000298-ET



CT contrast media injector

ulrichINJECT
CT *motion*™

Accessories

Product number

Power cable extension
5.0 m

XD 2068-00

Power supply cable

- | | |
|---|------------|
| ▪ Power supply cable CEE 7 Europe 2.0 m | XD 2068-01 |
| ▪ Power supply cable BS1363 GB 2.0 m | XD 2068-02 |
| ▪ Power supply cable GB2099 CN 2.0 m | XD 2068-03 |
| ▪ Power supply cable NBR14136 BR 2.5 m | XD 2068-04 |
| ▪ Power supply cable SANS164 RSA 1.5 m | XD 2068-05 |
| ▪ Power supply cable NEMA5-15 US 3.0 m | XD 2068-06 |
| ▪ Power supply cable SEV Type 12 CH 2.5 m | XD 2068-07 |
| ▪ Power supply cable CEI 23-50 ITA 1.5 m | XD 2068-08 |
| ▪ Power supply cable AS3112 AUS 2.0 m | XD 2068-09 |

Disposables

Product number

Pump tubing
24 h PU 80 items

XD 8003



Patient tubing
PU 100 items

- | | |
|----------|---------|
| ▪ 150 cm | XD 2035 |
| ▪ 250 cm | XD 2040 |
| ▪ 320 cm | XD 2045 |



ulrichINJECT CT motion™

CT contrast media injector



Software options Product number

| | | |
|--|---------|---|
| Same patient | XD 8009 | Multiple examinations on a patient without changing patient tubing |
| CM substitution | XD 8010 | Manual change from contrast medium to NaCl during injection |
| Tandem | XD 8011 | Careful selection of a second contrast medium* |
| Start delay | XD 8012 | Injection begins after a preset delay time |
| Stopwatch | XD 8013 | Acoustic signal after the set time has elapsed |
| Elapsed time | XD 8014 | Display of time elapsed since the end of injection |
| SYNCopen | XD 8016 | CANopen connection (CAN Class 1,3 and 4) Interface between contrast media injector and CT scanner based on international CiA standards |
| ulrich medical RIS/PACS Interface | XD 8158 | Interface for simple and comprehensive integration of CT motion in your RIS/PACS system using the DICOM standard |

* see instructions for use CT motion™

CT and MRI contrast media injectors

XD 200x injectors**

Accessories

Product number

Waste bin set

Consisting of waste bin and waste bin holder

XD2302-SET



Tray set

Consisting of tray and tray holder

XD 2303-SET



NaCl rod set for NaCl pouch

XD 2315-SET



Riverside II

Heater for contrast media
50-200 ml

XD 2322



Charging station including STECA charger

Only lead acid battery
(Only for XD 2000 and XD 2004)

XD 2170-24/3
XD 2171-9AH



Bottle holder KM 2

right


XD 2300



Bottle holder KM 1


left

XD 2301

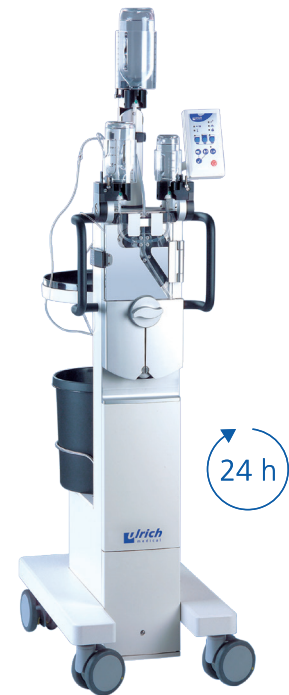

** mississippi™, missouri™, ohio tandem™, tennessee™, ohio M™

XD 200x injectors**

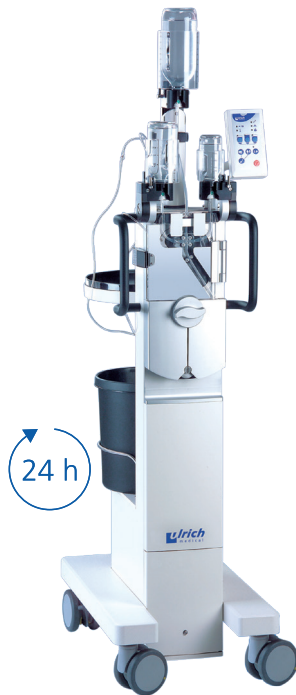

CT and MRI contrast media injectors

Accessories

Product number

Drip cup

XD 2304



Key for pump flap

Enables disassembly of the pump flap to make cleaning the roll pump easier.

XD 2305



Bottle holder NaCl swiveling

XD 2314



Standard guide tubes

- 20 ml, with locking device for bottles up to Ø 33 mm XD 2200-1
- 20 ml, with detent for bottles up to Ø 31 mm XD 2207
- 10 ml, with detent for bottles up to Ø 25 mm XD 2208
- 1000 ml, for bottles up to Ø 97 mm XD 2217



Special guide tubes

- 50 ml, Bracco ProHance, cap closure Ø 21 mm, for bottles up to Ø 44 mm XD 2205
- 20 ml, DOTAREM, with locking device, for bottles up to Ø 36 mm XD 2206
- 50 ml, MULTIHANCE, DIN for MRI, for bottles up to Ø 50 mm XD 2209



DIN guide tubes

- 100 ml, DIN for bottles up to Ø 50 mm XD 553025501
- 150/250 ml, DIN for bottles up to Ø 67 mm XD 553025565
- 500 ml, DIN for bottles up to Ø 79 mm XD 2267



EURO guide tubes

- 150/250 ml, EURO for bottles up to Ø 69 mm XD 553025503
- 500 ml, EURO for bottles up to Ø 87 mm XD 2268
- 125 ml, EURO for bottles up to Ø 55 mm XD 553025569



** mississippi™, missouri™, ohio tandem™, tennessee™, ohio M™

CT and MRI contrast media injectors

XD 200x injectors**

Accessories

Product number

Power cable extension
5.0 m

XD 2068-00 IEC

Power supply cable (Only for XD 2001
XD 2002 and XD 2003)


- | | |
|---|------------|
| ▪ Power supply cable CEE 7 Europe 2.0 m | XD 2068-01 |
| ▪ Power supply cable BS1363 GB 2.0 m | XD 2068-02 |
| ▪ Power supply cable GB2099 CN 2.0 m | XD 2068-03 |
| ▪ Power supply cable NBR14136 BR 2.5 m | XD 2068-04 |
| ▪ Power supply cable SANS164 RSA 1.5 m | XD 2068-05 |
| ▪ Power supply cable NEMA5-15 US 3.0 m | XD 2068-06 |
| ▪ Power supply cable SEV Type 12 CH 2.5 m | XD 2068-07 |
| ▪ Power supply cable CEI 23-50 ITA 1.5 m | XD 2068-08 |
| ▪ Power supply cable AS3112 AUS 2.0 m | XD 2068-09 |

Disposables

Product number

Pump tubing
24 h, PU 80 items

XD 2020



Patient tubing

PU 100 items

- | | |
|----------|---------|
| ▪ 120 cm | XD 2030 |
| ▪ 150 cm | XD 2035 |
| ▪ 250 cm | XD 2040 |
| ▪ 320 cm | XD 2045 |




Reservoir

24 h, PU 20 items


For the use of standard contrast media containers, scanbags, pre-filled, hand-held contrast media syringes, contrast media bottles with Luer lock

XD 2019

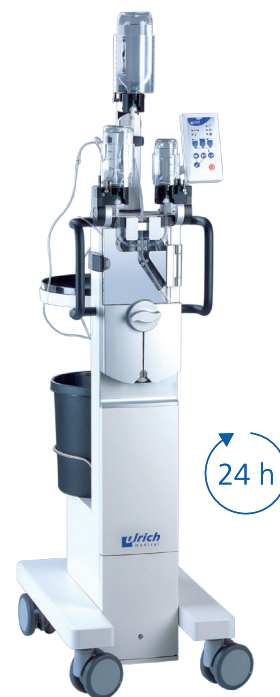

** mississippi™, missouri™, ohio tandem™, tennessee™, ohio M™

XD 200x injectors**

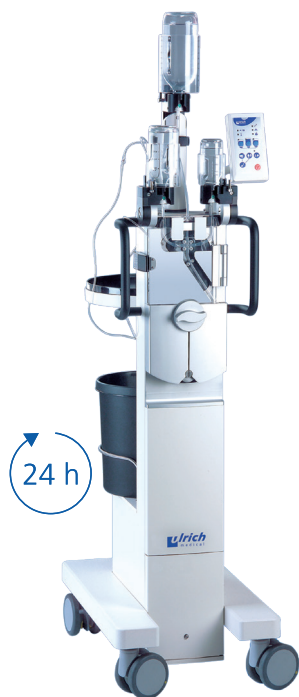

CT and MRI contrast media injectors

Software options Product number

| Software options | Product number | Description |
|------------------|----------------|--|
| Test bolus | XDTESTBOLE | Injection of a contrast media test bolus to determine the patient's circulation time |
| Same patient | XDSAMEPATIEN | Multiple examinations on a patient without changing patient tubing |
| Last patient | XDLASTPATIEN | Automatic filling of the tubing system with NaCl |
| Stopwatch | XDSTOPWATCH | Acoustic signal after the set time has elapsed |
| Tandem | XDTANDEM | Careful selection of a second contrast medium (only mississippi and missouri) |

** mississippi™, missouri™, ohio tandem™, tennessee™, ohio M™

Overview of product numbers

Accessories

PU

ulricheasyINJECT Max 3™ and Max 2M™

| | | |
|----------------|--|-----------|
| XD 10500 | Convenience package, consisting of waste bin, tray and media rod | 1 item |
| XD 10740 | Drip cup | 5 items |
| XD 10741 | Adapter ring for small bottles, for contrast media bottles with bottle neck diameter of 21 mm for adapting to an Easy-Click-Cassette holder I contrast media spike | 100 items |
| XD 2068-00 IEC | Power extension cable, 5.0 m | 1 item |
| XD 2068-01 | Power supply cable CEE 7 Europe 2.0 m | 1 item |
| XD 2068-02 | Power supply cable BS1363 GB 2.0 m | 1 item |
| XD 2068-03 | Power supply cable GB2099 CN 2.0 m | 1 item |
| XD 2068-04 | Power supply cable NBR14136 BR 2.5 m | 1 item |
| XD 2068-05 | Power supply cable SANS164 RSA 1.5 m | 1 item |
| XD 2068-06 | Power supply cable NEMA5-15 US 3.0 m | 1 item |
| XD 2068-07 | Power supply cable SEV Type 12 CH 2.5 m | 1 item |
| XD 2068-08 | Power supply cable CEI 23-50 ITA 1.5 m | 1 item |
| XD 2068-09 | Power supply cable AS3112 AUS 2.0 m | 1 item |
| SP001612-ET | Bottle holder multiuse | 1 item |
| SP002808-ET | Pair of holding arms | 1 item |

ulrichINJECT CT motion™

| | | |
|-------------|---|---------|
| XD 2068-00 | Power extension cable, 5.0 m | 1 item |
| XD 2068-01 | Power supply cable CEE 7 Europe 2.0 m | 1 item |
| XD 2068-02 | Power supply cable BS1363 GB 2.0 m | 1 item |
| XD 2068-03 | Power supply cable GB2099 CN 2.0 m | 1 item |
| XD 2068-04 | Power supply cable NBR14136 BR 2.5 m | 1 item |
| XD 2068-05 | Power supply cable SANS164 RSA 1.5 m | 1 item |
| XD 2068-06 | Power supply cable NEMA5-15 US 3.0 m | 1 item |
| XD 2068-07 | Power supply cable SEV Type 12 CH 2.5 m | 1 item |
| XD 2068-08 | Power supply cable CEI 23-50 ITA 1.5 m | 1 item |
| XD 2068-09 | Power supply cable AS3112 AUS 2.0 m | 1 item |
| XD 8018 | Waste bin | 1 item |
| XD 8021 | Tray | 1 item |
| XD 8118 | Protective cap for particle filter holder | 1 item |
| XD 8090 | Tube insertion device | 1 item |
| XD 8163 | NaCl rod | 1 item |
| XD 10740 | Drip cup | 5 items |
| SP000298-ET | Bottle holder | 1 item |

Please send orders to:
injectors@ulrichmedical.com
 Phone +49 731 9654-0
 Fax +49 731 9654-199

Overview of product numbers

Accessories

PU

XD 200x injectors**

| | | |
|----------------|--|--------|
| XD 2170-24/3 | Charging station including STECA charger | 1 item |
| XD 2171-9AH | Lead acid battery | 1 item |
| XD 2200-1 | Standard guide tube, 20 ml, with locking device | 1 item |
| XD 2205 | Special guide tube, 50 ml, Bracco ProHance, cap closure Ø 21 mm, for bottles up to Ø 44 mm | 1 item |
| XD 2206 | Special guide tube, 20 ml, DOTAREM, with locking device, for bottles up to Ø 36 mm | 1 item |
| XD 2207 | Standard guide tube, 20 ml, with detent for bottles up to Ø 31 mm | 1 item |
| XD 2208 | Standard guide tube, 10 ml, with detent for bottles up to Ø 25 mm | 1 item |
| XD 2209 | Special guide tube, 50 ml, MULTIHANCE, DIN for MRI, for bottles up to Ø 50 mm | 1 item |
| XD 2217 | Standard guide tube, 1000 ml, for bottles up to Ø 97 mm | 1 item |
| XD 2267 | DIN guide tube, 500 ml, DIN for bottles up to Ø 79 mm | 1 item |
| XD 2268 | EURO guide tube, 500 ml, EURO for bottles up to Ø 87 mm | 1 item |
| XD 2300 | Bottle holder, contrast media 2 right | 1 item |
| XD 2301 | Bottle holder, contrast media 1 left | 1 item |
| XD 2302-SET | Waste bin set, consisting of waste bin and waste bin holder | 1 item |
| XD 2303-SET | Tray set, consisting of tray and tray holder | 1 item |
| XD 2304 | Drip cup | 1 item |
| XD 2305 | Key for pump flap Enables disassembly of the pump flap to make cleaning the roll pump easier. | 1 item |
| XD 2314 | Bottle holder NaCl, swiveling | 1 item |
| XD 2315 set | NaCl rod set for NaCl pouch | 1 item |
| XD 2322 | Riverside II | 1 item |
| XD 2068-00 IEC | Power extension cable, 5.0 m | 1 item |
| XD 2068-01 | Power supply cable CEE 7 Europe 2.0 m | 1 item |
| XD 2068-02 | Power supply cable BS1363 GB 2.0 m | 1 item |
| XD 2068-03 | Power supply cable GB2099 CN 2.0 m | 1 item |
| XD 2068-04 | Power supply cable NBR14136 BR 2.5 m | 1 item |
| XD 2068-05 | Power supply cable SANS164 RSA 1.5 m | 1 item |
| XD 2068-06 | Power supply cable NEMA5-15 US 3.0 m | 1 item |
| XD 2068-07 | Power supply cable SEV Type 12 CH 2.5 m | 1 item |
| XD 2068-08 | Power supply cable CEI 23-50 ITA 1.5 m | 1 item |
| XD 2068-09 | Power supply cable AS3112 AUS 2.0 m | 1 item |
| XD 553025501 | DIN guide tube, 100 ml, DIN for bottles up to Ø 50 mm | 1 item |
| XD 553025503 | EURO guide tube, 150/250 ml, EURO for bottles up to Ø 69 mm | 1 item |
| XD 553025565 | DIN guide tube, 150/250 ml, DIN for bottles up to Ø 67 mm | 1 item |
| XD 55025569 | EURO guide tube, 125 ml, EURO for bottles up to Ø 55 mm | 1 item |

** mississippi™, missouri™, ohio tandem™, tennessee™, ohio M™

Please send orders to:
injectors@ulrichmedical.com
 Phone +49 731 9654-0
 Fax +49 731 9654-199

Overview of product numbers

Disposables

PU

ulricheasyINJECT Max 3™

| | | |
|----------|--|-----------|
| XD 10710 | Easy-Click-Cassette Max 3™, 24 h, with holder s for contrast media bottles with a bottle neck diameter of 21 mm | 40 items |
| XD 10711 | Easy-Click-Cassette Max 3™, 24 h, with holder l for contrast media bottles with a bottle neck diameter of 33 mm | 40 items |
| XD 10716 | Easy-Click-Cassette Max 3™ – flex, 24 h | 40 items |
| XD 10704 | Spike for CT (CM/NaCl), MRI (NaCl) | 30 items |
| XD 10705 | Spike for MRI (CM) – holder l, with holder l for contrast media bottles with a bottle neck diameter of 33 mm | 30 items |
| XD 10706 | Spike for MRI (CM) – holder s, with holder s for contrast media bottles with a bottle neck diameter of 21 mm | 30 items |
| XD 10701 | Patient tubing 250 cm, 2 check valves | 100 items |
| XD 10702 | Patient tubing 320 cm, 2 check valves | 100 items |
| XD 10707 | Patient tubing system, consisting of XD 10703 patient tubing connector and patient tubing 320 cm (XD 2045) for the use of pre-filled contrast media syringes | 50 items |

ulricheasyINJECT Max 2M™

| | | |
|----------|--|-----------|
| XD 10712 | Easy-Click-Cassette Max 2M™, 24 h, with holder s for contrast media bottles with a bottle neck diameter of 21 mm | 40 items |
| XD 10713 | Easy-Click-Cassette Max 2M™, 24 h, with holder l for contrast media bottles with a bottle neck diameter of 33 mm | 40 items |
| XD 10717 | Easy-Click-Cassette Max 2M™ – flex, 24 h | 40 items |
| XD 10704 | Spike for CT (CM/NaCl), MRI (NaCl) | 30 items |
| XD 10705 | Spike for MRI (CM) – holder l, with holder l for contrast media bottles with a bottle neck diameter of 33 mm | 30 items |
| XD 10706 | Spike for MRI (CM) – holder s, with holder s for contrast media bottles with a bottle neck diameter of 21 mm | 30 items |
| XD 10701 | Patient tubing 250 cm, 2 check valves | 100 items |
| XD 10702 | Patient tubing 320 cm, 2 check valves | 100 items |
| XD 10707 | Patient tubing system, consisting of patient tubing connector (XD 10703) and patient tubing 320 cm (XD 2045) for the use of pre-filled contrast media syringes | 50 items |

ulrichINJECT CT motion™

| | | |
|---------|---------------------------------------|-----------|
| XD 8003 | Patient tubing, 24 h | 80 items |
| XD 2035 | Patient tubing 150 cm, 2 check valves | 100 items |
| XD 2040 | Patient tubing 250 cm, 2 check valves | 100 items |
| XD 2045 | Patient tubing 320 cm, 2 check valves | 100 items |

XD 200x injectors**

| | | |
|---------|--|-----------|
| XD 2020 | Patient tubing, 24 h | 80 items |
| XD 2030 | Patient tubing 120 cm, 2 check valves | 100 items |
| XD 2035 | Patient tubing 150 cm, 2 check valves | 100 items |
| XD 2040 | Patient tubing 250 cm, 2 check valves | 100 items |
| XD 2045 | Patient tubing 320 cm, 2 check valves | 100 items |
| XD 2019 | Reservoir, 24 h, for the use of standard contrast media containers, scanbags, pre-filled, hand-held contrast media syringes, contrast media bottles with Luer lock | 20 items |

** mississippi™, missouri™, ohio tandem™, tennessee™, ohio M™

Overview of product numbers

Software options

ulricheasyINJECT Max 3™

| | |
|----------|--|
| XD 10600 | Max 3™ software package consisting of CM-Select, Same patient and Vein-check |
| XD 10630 | Same patient |
| XD 10640 | CM-Select |
| XD 10650 | Vein-check |

ulricheasyINJECT Max 2M™

| | |
|----------|--|
| XD 10610 | Max 2M™ software package consisting of Same patient and Vein-check |
| XD 10630 | Same patient |
| XD 10650 | Vein-check |

ulrichINJECT CT motion™

| | |
|---------|-------------------------------------|
| XD 8009 | Same patient |
| XD 8010 | CM substitution |
| XD 8011 | Tandem |
| XD 8012 | Start delay |
| XD 8013 | Stopwatch |
| XD 8014 | Elapsed time |
| XD 8016 | SYNCopen – CANopen Class 1, 3 and 4 |
| XD 8158 | ulrich medical RIS/PACS Interface |

XD 200x series*

| | |
|--------------|--|
| XDLASTPATIEN | Last patient |
| XDSAMEPATIEN | Same patient |
| XDSTOPWATCH | Stopwatch |
| XDTANDEM | Tandem (only mississippi and missouri) |
| XDTESTBOLE | Test bolus |

Supporting member of the German Society for Hospital Hygiene (Deutsche Gesellschaft für Krankenhaushygiene e.V.)

Over a Century
of Innovation

* missouri™, mississippi™, ohio M™, ohio tandem™ and tennessee™



ulrich GmbH & Co. KG | Buchbrunnenweg 12 | 89081 Ulm | Germany
Phone: +49 731 9654-0 | Fax: +49 731 9654-199
injectors@ulrichmedical.com | www.ulrichmedical.com